

Concise Communication

Protein detection by fluorescence of manually cleaned high-speed dental handpieces

Fábio B. Souza DDS, MSc, PhD¹, Camila Q.M. Bruna PhD² , Rosa A.B. Mesiano PhD³ , Regina M.B. Cicarelli PhD⁴ , David Perrett PhD⁵ and Kazuko U. Graziano PhD⁶

¹Department of Prosthodontics and Oral Facial Surgery, Federal University of Pernambuco. Recife, Pernambuco, Brazil, ²Medical Surgical Nursing Department, Escola de Enfermagem, Universidade de São Paulo, São Paulo, Brazil, ³National Health Surveillance Agency, Federal Government, Brasília, Brazil, ⁴Department of Biological Sciences, School of Pharmacy, State University of São Paulo, Araraquara, Brazil, ⁵Queen Mary, University of London, William Harvey Research Institute, London, United Kingdom and ⁶Medical Surgical Nursing Department, Escola de Enfermagem, Universidade de São Paulo, São Paulo, Brazil

Abstract

We analyzed the effectiveness of manual cleaning protocols performed on high-speed dental handpieces, using protein identification by fluorescence. Although one protocol was able to lower the amount of protein, >40% of the handpieces showed amounts of residual protein at unacceptable levels.

(Received 28 October 2021; accepted 2 February 2022; electronically published 7 April 2022)

Dental clinical practice often requires the use of high-speed rotation handpieces, which are complex medical equipment, representing a challenge for suitable cross-contamination control practices. The cross contamination from microorganisms inside the handpieces could be expelled during the use of the equipment.¹ Thus, handpieces require sterilization by methods that use heat (ie, autoclave) after each use.¹ As much as sterilization is the method of choice, the presence of organic matter (proteins) remaining on the surfaces of health products resulting from an inadequate cleaning process limits the effectiveness of sterilization.² In addition, organic material can protect microorganisms by acting as a physical barrier,³ impairing subsequent sterilization steps, as well as favoring the formation of biofilms. Thus, removal of biomaterial is necessary for sterilization to be effective.

Even with the development of automated cleaning devices, manually cleaning dental handpieces is still the most frequent cleaning method in oral health services. In these situations, visual inspection by magnifying glasses has been the method adopted to validate the cleaning process. But is this practice enough to provide safe levels of cleanliness? One study answered this question for neurosurgical instruments using the in situ protein detection system (ProReveal, Synoptics Health, UK), capable of quantifying the protein levels by fluorescence.⁴ The use of this innovative technology in dentistry could be valuable for measuring the protein residue accumulated on dental handpieces. In this study, we conducted an exploratory analysis of the effectiveness of manually cleaning the external surface of high-speed dental handpieces using protein identification by fluorescence.

Author for correspondence: Fábio B. Barbosa de Souza, DDS, MSc, PhD, E-mail: Fabio.souza@ufpe.br

Cite this article: Souza FB, *et al.* (2023). Protein detection by fluorescence of manually cleaned high-speed dental handpieces. *Infection Control & Hospital Epidemiology*, 44: 840–842, <https://doi.org/10.1017/ice.2022.36>

Methods

In this cross-sectional, exploratory study, data collection took place in 3 dental clinics with at least 5 dental units for outpatient care. The sample consisted of at least 3 different high-speed handpieces from each study site. The high-speed handpieces were used in clinical procedures such as restorations and endodontic treatments. Visits were made to the service locations to analyse the cleaning process.

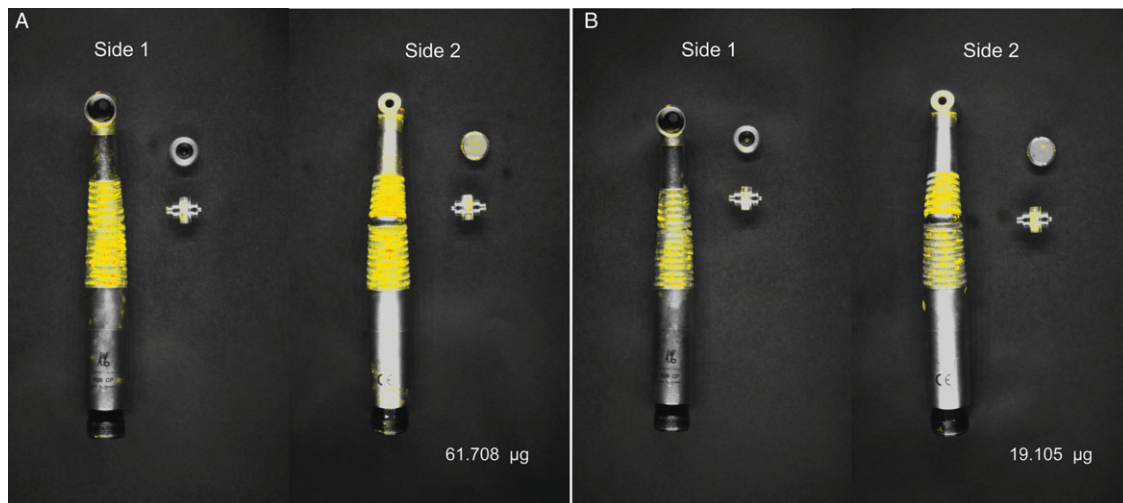
Proteins on the high-speed handpieces were identified after completion of the cleaning method adopted in each health service (group A) according to their choice, and after the adapted CDC-USA cleaning protocol⁵ (group B). This protocol was carried out by trained personnel as follows: (1) activation of the air and/or water lines of the high-speed handpieces 30 seconds; (2) wrapping the handpiece with gauze soaked in enzymatic detergent; (3) scrubbing the gauze soaked with enzymatic detergent (Indazyme7 Max/Indalabor – Brazil) over the entire handpiece body (30 seconds); (4) rinsing the handpiece under running tap water; (5) visual inspection; and (6) drying the handpiece.

The protein detection equipment (ProReveal, Synoptics Health/UK) was used according to the manufacturer's instructions. The equipment issued a report after each reading with a digital image record, protein quantification, and the cleaning "status" of the analyzed instrument. The study utilized the criterion adopted by Technical Memorandum 01-01 of the UK Department of Health,⁶ which indicates that the upper limit of acceptable contamination of proteins after processing is 5 µg of protein on one side of an instrument.

The 3 parts of each handpiece (body, end cap, and bearing) were analyzed at the same time, and 2 fluorescence readings were performed: 1 reading for each side of the high-speed handpiece. Thus, each handpiece was considered to have a "passed" status when the sum of the analyses on each side of the high-speed handpiece was ≤10 µg protein residue. The results were subjected to statistical

Table 1. Residual Protein Levels (μg) in High-Speed Handpieces After the Cleaning Method Adopted by the Studied Clinics (Moment 1) and After the Cleaning Protocol of the Adapted CDC-USA (Moment 2), São Paulo, 2019

Handpiece/Clinic	Group A				Group B			
	Side 1	Side 2	Total	Status	Side 1	Side 2	Total	Status
1/A	2.32	0.909	3.229	Passed	0.675	0.493	1.168	Passed
2/A	2.402	4.461	6.863	Passed	0.516	2.968	3.484	Passed
3/A	6.798	4.844	11.642	Failed	0.241	0	0.241	Passed
4/A	2.233	8.971	11.204	Failed	0.915	6.063	6.978	Passed
5/A	45.731	67.35	113.081	Failed	47.235	63.976	111.211	Failed
6/B	2.343	0.986	3.329	Passed	0.347	0.396	0.743	Passed
7/B	10.949	8.391	19.34	Failed	3.888	4.437	8.325	Passed
8/B	18.104	23.837	41.941	Failed	11.646	16.567	28.213	Failed
9/B	2.974	4.16	7.134	Passed	1.681	3.295	4.976	Passed
10/B	16.236	17.114	33.35	Failed	5.061	7.354	12.415	Failed
11/B	1.282	2.597	3.879	Passed	0.241	0.815	1.056	Passed
12/C	14.699	26.765	41.464	Failed	12.281	22.773	35.054	Failed
13/C	74.323	85.783	160.106	Failed	43.592	59.766	103.358	Failed
14/C	27.292	34.416	61.708	Failed	7.009	12.096	19.105	Failed

**Figure 1** Images obtained using ProReveal from the 14/C high-speed handpiece showing the protein accumulation (highlighted in yellow) in Group A (after the cleaning adopted in each health service), and Group B (after the cleaning protocol of the adapted CDC-USA). It is observed that the grooves on the handpiece surface favour protein content accumulation.

analysis using SPSS version 23 software (IBM, Armonk, NY). We adopted a significance level of 5% to verify whether there was a difference between the cleaning methods studied, considering the average protein values measured.

Results

The decontamination procedures for handpieces adopted by all clinics consisted of applying 70% ethyl alcohol solution on the external surface of the high-speed handpieces under friction with gauze or absorbent paper for an indefinite period, however, for no longer than 30 seconds.

Protein quantification was performed in 14 high-speed handpieces, and the results are shown in Table 1. The average protein quantification in high-speed handpieces was $37.02 \mu\text{g}$ (group A) and $24.02 \mu\text{g}$ (group B). The proportion of devices that passed the test after the application of each cleaning protocol was 35.7% (group A) and 57.1% (group B). The paired Wilcoxon test for the comparison between the groups indicated a statistically significant reduction at the 5% level ($P < .001$) after cleaning.

Figure 1 illustrates the images captured by the ProReveal equipment, in which the protein contaminated areas are visualized in yellow.

Discussion

This study leads to a worrying finding that methods used to clean high-speed dental handpieces are failing to remove protein, thereby allowing potential cross contamination since these devices are used repeatedly on different patients. All high-speed handpieces exhibited a reduction in the amount of protein residue after the adapted CDC cleaning protocol was used. However, this process was not enough to guarantee levels $>10 \mu\text{g}$ protein residue for 42.9% of the samples.

The presence of residual debris in handpieces is a constant risk. Because cleaning is a fundamental step for sterilization success, the method that detects and quantifies proteins by fluorescence was able to provide accurate data regarding high-speed handpieces. Importantly, the maximum protein limit adopted for recording the cleaning status ($\leq 5 \mu\text{g}$) accounted for a strict cleaning criterion directed to instruments used in sterile tissues, such as those used in neurosurgical procedures. Additional contamination concern is related to prions in these situations, which are transmissible and infectious protein particles that do not contain nucleic acid.⁷ These particles are related to specific neurological degenerative diseases.⁸ However, there is no consensus on the acceptable protein level in the context of using high-speed handpieces in dental practice.

When considering the high-speed handpiece as an instrument, which is part of the daily routine of dental health services, it can be fit into the criterion adopted by the German Society for Hospital Hygiene⁹ in which the safe limit of protein content after cleaning should be $\leq 80 \mu\text{g}$. Thus, when adopting this criterion, 2 handpieces in the study (5A and 13C) would have been unfit for use after sterilization. These handpieces would likely have conferred high contamination risks during clinical use.

Some factors may have contributed to the permanence of surface proteins even after cleaning. One is related to the external design of the equipment that functions as a shelter for proteins to accumulate (Fig. 1). Another aspect is the fact that many manufacturers contraindicate both immersion in detergent solutions and automated cleaning. The CDC cleaning protocol (group B) was adapted for the present study to overcome this limitation. However, the data presented here reveal the weakness in applying the high-speed handpiece manual cleaning in group B protocol. In addition, ethyl alcohol performance on high-speed handpiece surfaces has proven to be an inadequate practice without prior cleaning.¹⁰

In conclusion, the manual cleaning protocol used by the 3 dental services providers included in the study was ineffective in reliably achieving a postcleaning protein level of $\leq 10 \mu\text{g}$ protein residue. The adapted CDC-USA protocol was able to lower the amount of residual protein. However, in $>40\%$ of the handpieces, the amounts of residual protein remained $>10 \mu\text{g}$.

Acknowledgments. We thank Cicarelli Surgical Instruments company for providing the ProReveal equipment (Synoptics Health, UK) to conduct the analysis.

Financial support. This study was financed in part by the Coordenação de Aperfeiçoamento de Pessoal de Nível Superior–Brasil (CAPES) (finance code 001).

Conflicts of interest. We confirm that all authors have no conflict of interest to declare.

References

1. Kohn WG, Harte JA, Malvitz DM, *et al.* Guidelines for infection control in dental health care settings—2003. *J Am Dent Assoc* 2004;135:33–47.
2. Rutala WA, Weber DJ. Disinfection, sterilization, and antisepsis: an overview. *Am J Infect Control* 2019;47S:A3–A9.
3. Muscarella LF. Sterilizing dental equipment. *Nat Med* 1995;1:1223–1225.
4. Smith A, Winter S, Lappin D, *et al.* Reducing the risk of iatrogenic Creutzfeldt-Jakob disease by improving the cleaning of neurosurgical instruments. *J Hosp Infect* 2018;100(3):e70–e76.
5. Alvarenga CF, Reis C, Tipple AFV, Paiva EMM, Sasamoto SAA. Efetividade de um protocolo de processamento na esterilização de canetas de alta rotação em autoclave gravitacional. *Rev Eletr Enf* 2011;13:560–565.
6. Advisory Committee on Dangerous Pathogens' Transmissible Spongiform Encephalopathy (ACDP TSE) Subgroup. Transmissible spongiform encephalopathy agents: safe working and the prevention of infection: Annex C—General principles of decontamination and waste disposal. UK government website. https://assets.publishing.service.gov.uk/government/uploads/system/uploads/attachment_data/file/427855/Annex_C_v3.0.pdf. Accessed October 6, 2020.
7. Azarpazhooh A, Leake JL. Prions in dentistry—what are they, should we be concerned, and what can we do? *J Can Dent Assoc* 2006;72:53–60.
8. Jayanthi P, Thomas P, Bindhu P, Krishnapillai R. Prion diseases in humans: oral and dental implications. *N Am J Med Sci* 2013;5:399–403.
9. Carter A, Biering, Gebel J. Zentral sterilisation—Annex 9: acceptance criteria for assessment of cleaning efficacy. Sociedad Científica de Enfermeras Especialistas en Esterilización website. http://socienee.com/archivos/manual_limpieza_dispositivos_medicos.pdf. Accessed October 8, 2021.
10. Pinto FM, Bruna CQ, Camargo TC, *et al.* The practice of disinfection of high-speed handpieces with 70% w/v alcohol: an evaluation. *Am J Infect Control* 2017;45(1):e19–e22.